



Smart maltose microneedle for blood sampling fabricated by stepwise controlled drawing

Puttaswamy, S., Fishlock, S., Steele, D., Navarro-Paredes, C., Lubarsky, G., Raj, S., Lee, C., & McLaughlin, J. (Accepted/In press). *Smart maltose microneedle for blood sampling fabricated by stepwise controlled drawing*. Poster session presented at IEEE EMBC 2019, BERLIN, BERLIN, Germany.

[Link to publication record in Ulster University Research Portal](#)

Publication Status:

Accepted/In press: 14/05/2019

Document Version

Publisher's PDF, also known as Version of record

General rights

Copyright for the publications made accessible via Ulster University's Research Portal is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

The Research Portal is Ulster University's institutional repository that provides access to Ulster's research outputs. Every effort has been made to ensure that content in the Research Portal does not infringe any person's rights, or applicable UK laws. If you discover content in the Research Portal that you believe breaches copyright or violates any law, please contact pure-support@ulster.ac.uk.

Smart maltose microneedle for blood sampling fabricated by stepwise controlled drawing

Srinivasu Valagerahally Puttaswamy^a, Sam Jeffery Fishlock^a, David Steele^a, Cesar Navarro^a, Gennady Lubarsky^a, Shasidran Raj^a, Chengkuo Lee^{b,c} and James McLaughlin^a

Abstract— The present work designed to fabricate, characterize and use maltose microneedles for blood sampling application. Sugar microneedle was fabricated by drawing lithography technique and investigated for mechanical properties and required dimensions. Microneedle was subjected to plasma treatment to enhance hydrophilicity for rapid transport of bio sample.

I. INTRODUCTION

Routine blood sampling is crucial for medical diagnosis to understand, prevent, and treatment of specific disease. It can provide critical information such as level of blood components, specific biomarker and improvements after treatment[1]. Many previous studies have been focussed on employing microneedles for body fluid sampling, highlighting its advantages compared to conventional hypodermic needles [2]. Biocompatible microneedles are fabricated using various methods. Maltose is a safe material for both body fluid sampling and drug delivery application[3].

II. METHODS

Microneedle is fabricated by inexpensive, simple stepwise drawing lithography technique[4]. The fabricated microneedle was investigated for mechanical properties to ensure it is strong enough to perforate skin when employed for blood sampling.

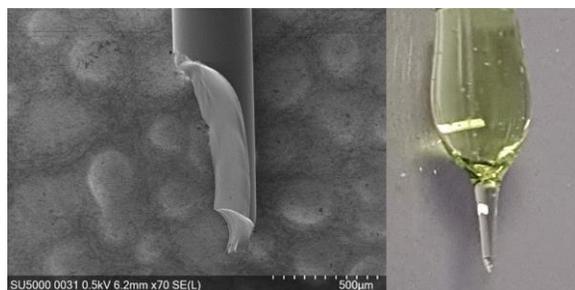


Figure 1. Maltose microneedles with SEM image showing tip of microneedle.

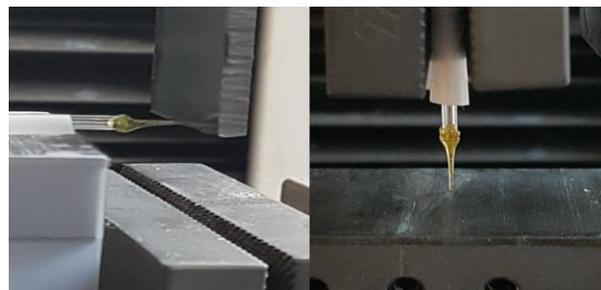


Figure 2. Maltose microneedles investigated for mechanical properties.

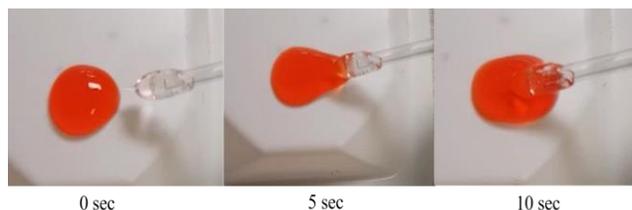


Figure 3. Superhydrophilic behaviour of maltose microneedle.

III. DISCUSSION & CONCLUSION

Super hydrophilic properties of plasma treated microneedle is demonstrated as shown in Figure 3. Microneedle integrated with glass capillary tube was brought in contact with the liquid. With in a short span of 10 seconds, the liquid sample is drawn from tip towards base of microneedle demonstrating its suitability for proposed application. The developed microneedle can be conveniently integrated with lateral flow device for biomedical diagnostic application.

ACKNOWLEDGMENT

This work was supported by funding under the Invest Northern Ireland and the European Union's INTERREG VA Programme, managed by the Special EU Programmes Body (SEUPB) under the Connected Health Innovation Centre (CHIC) competence center

REFERENCES

- [1]P. Xue, L. Zhang, Z. Xu, J. Yan, Z. Gu, and Y. Kang, "Blood sampling using microneedles as a minimally invasive platform for biomedical diagnostics," *Appl. Mater. Today*, vol. 13, pp. 144–157, 2018.
- [2]T. Miyano *et al.*, "Sugar micro needles as transdermic drug delivery system," *Biomed. Microdevices*, vol. 7, no. 3, pp. 185–188, 2005.
- [3]K. Takeuchi, N. Takama, B. Kim, K. Sharma, O. Paul, and P. Ruther, "Microfluidic chip to interface porous microneedles for ISF collection," *Biomed. Microdevices*, vol. 21, no. 1, p. 28, 2019.
- [4]K. Lee and H. Jung, "Drawing lithography for microneedles: a review of fundamentals and biomedical applications," *Biomaterials*, vol. 33, no. 30, pp. 7309–7326, 2012.

^aConnected Health Innovation Centre, Engineering Research Institute, Ulster University, Newtownabbey, United Kingdom

^bSingapore Institute for Neurotechnology, Centre for Life Sciences, National University of Singapore

^cDepartment of Electrical and Computer Engineering, National University of Singapore

email: srini@ulster.ac.uk